


**Patient Information**

**Patient ID :** 12345678  
**Name :** Lastname, Firstname  
 Birth Date : 09-Apr-1976  
 Professional : Yourname  
 Today's Date : 09-Aug-2020, 16:25:59

Street : Street  
 City : City  
 State/Prov. : Province A1B 2C3  
 Country : Canada  
 Phone : (519) 123-4567

**LEFT EAR**

**Verification SPLogram**

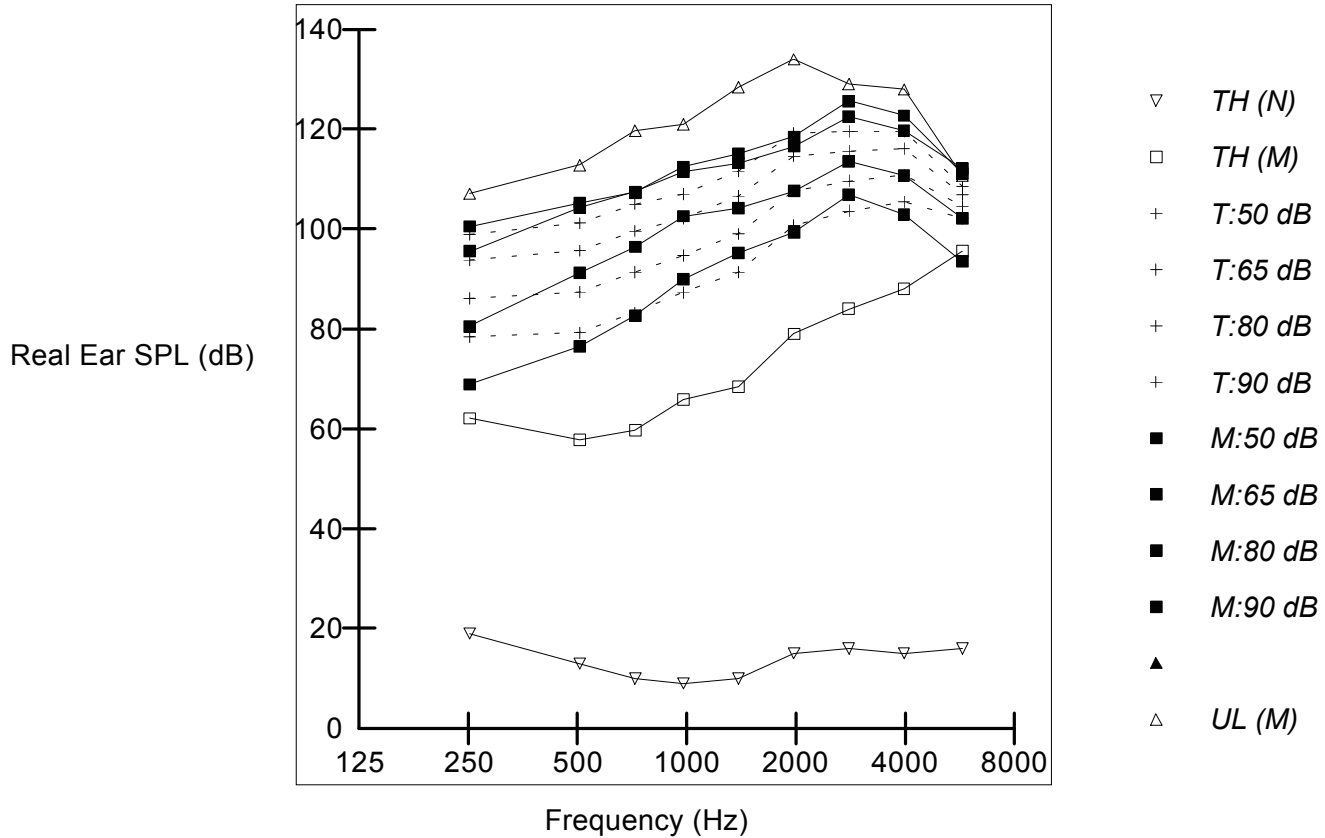

**HEARING AID RECOMMENDATION**

**LEFT EAR**

**Selection Method :** DSL [i/o]

HEARING AID

Style : BTE  
 Make :  
 Model :  
 Serial # :

EARMOLD

Type : SHELL  
 Tube : NORMAL #13  
 Bore : STANDARD #13  
 Vent : PRESSURE 1MM  
 Material : NEWSIL

OTHER

Transducer : ER3  
 HL to SPL : RECD  
 HA Style : BTE  
 Circuit : WDRC (fixed CR)  
 RE to 2cc : Measured

OTHER

Speech : Cox/Moore  
 Compr. Thresh : 50  
 Loudness : Predicted  
 Max. Out : Measured

	<u>.25</u>	<u>.50</u>	<u>.75</u>	<u>1.0</u>	<u>1.5</u>	<u>2.0</u>	<u>3.0</u>	<u>4.0</u>	<u>6.0</u>
SSPL-90	105	109	116	115	121	126	118	115	97
Full-On Gain (Reserve 10 dB)	29	28	32	33	36	43	42	42	35
User Gain (Input 65 dB)	19	18	22	23	26	33	32	32	25
Comp. Ratio	2.0	1.8	1.8	2.0	2.0	2.2	2.5	2.8	6.3